






4/22 FIG. 4

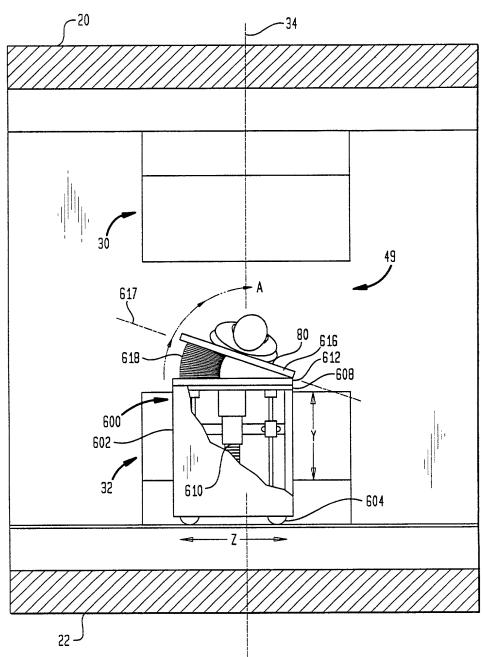


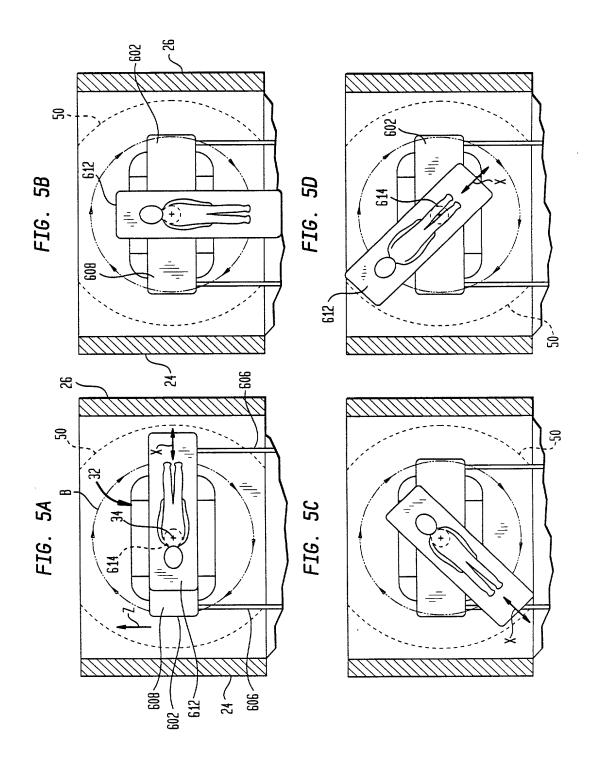

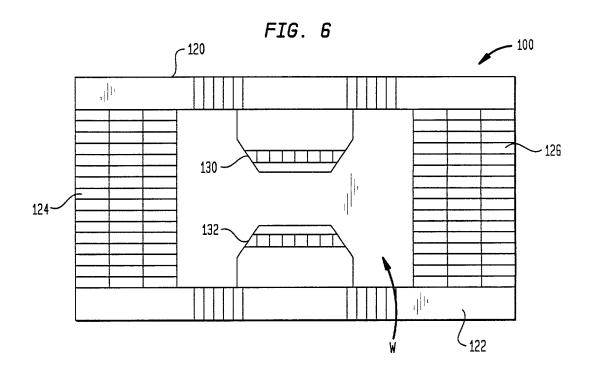

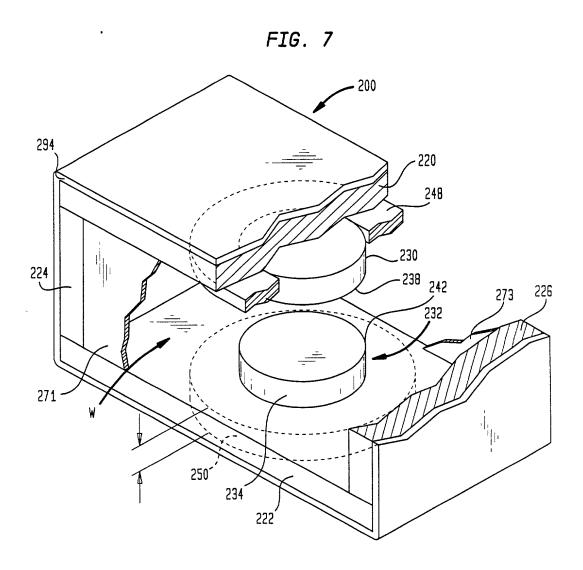

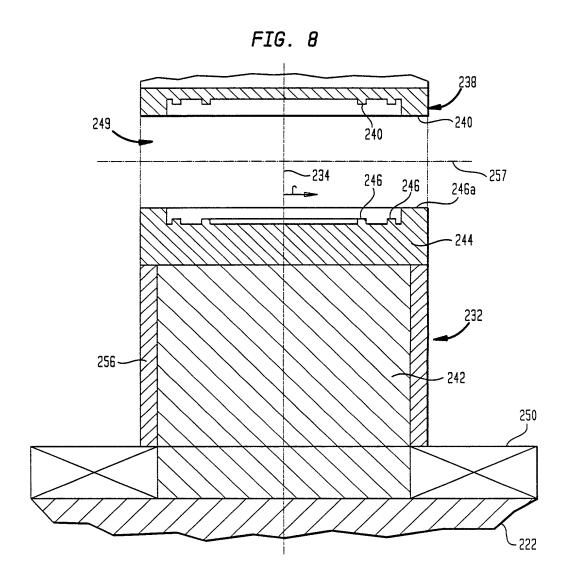

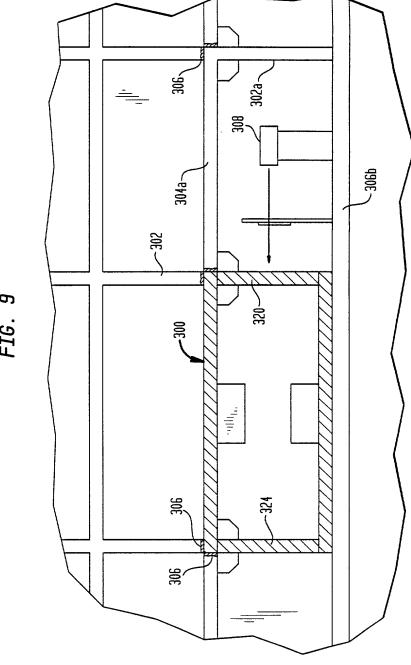

10/22

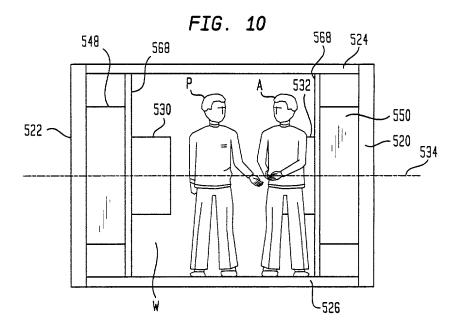


FIG. 11

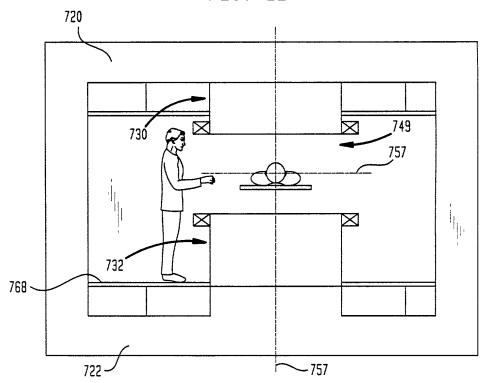
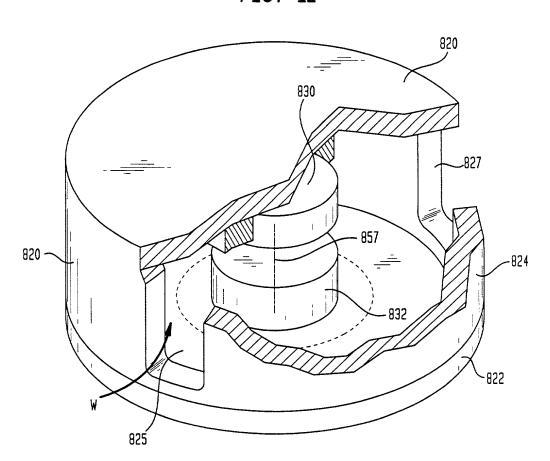
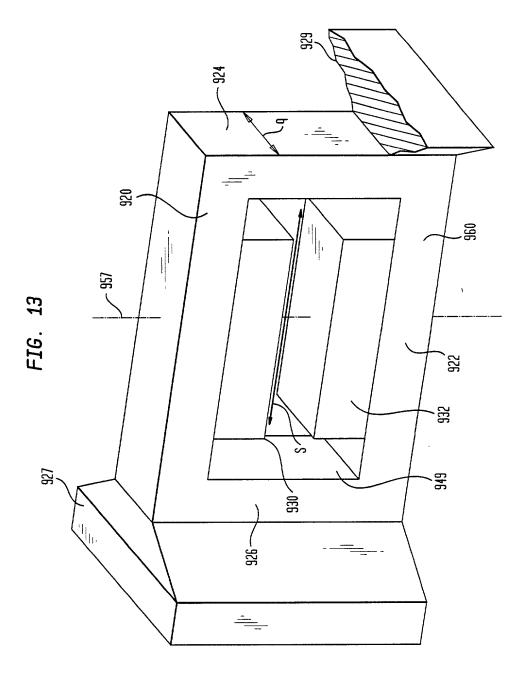
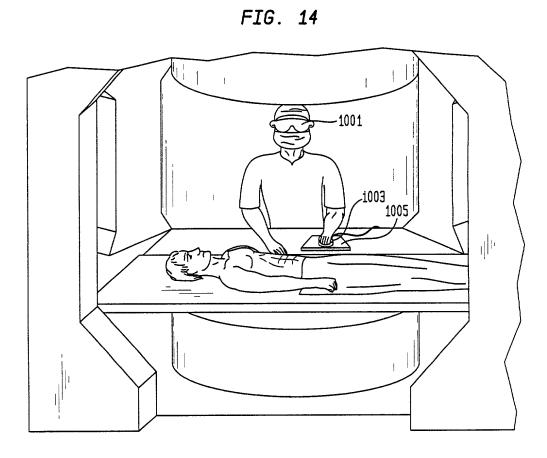


FIG. 12







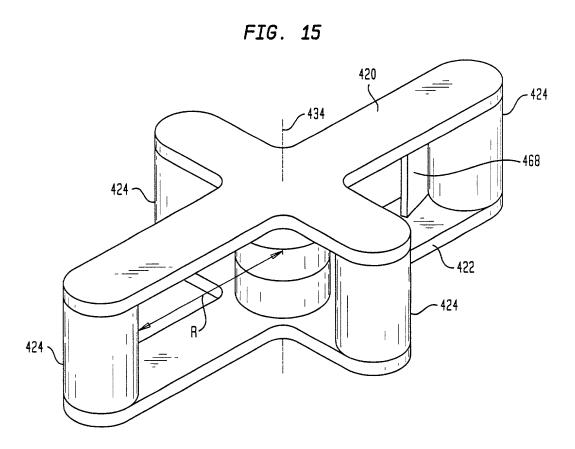
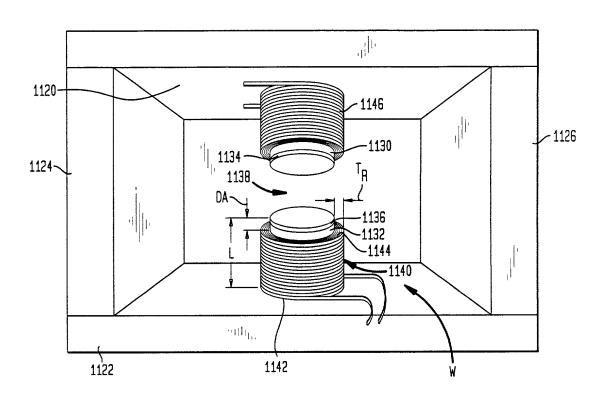


FIG. 16




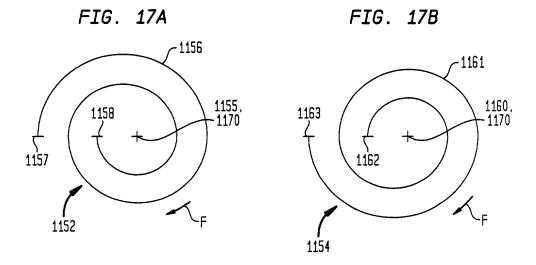


FIG. 17C

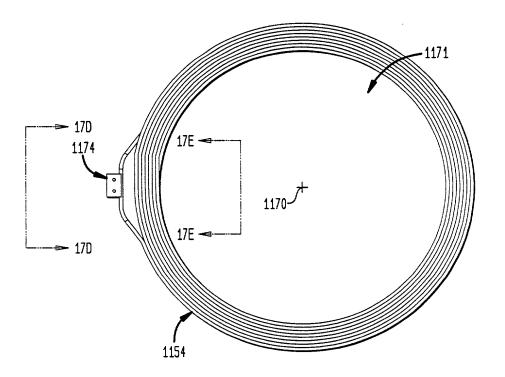

17/22 FIG. 17D

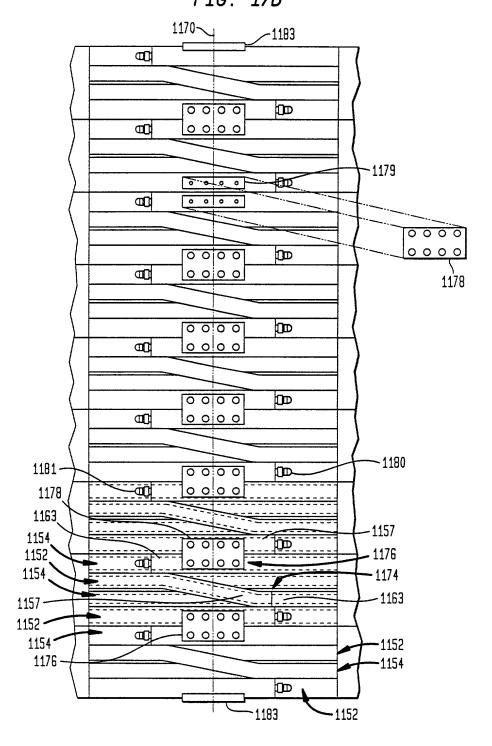


FIG. 17E



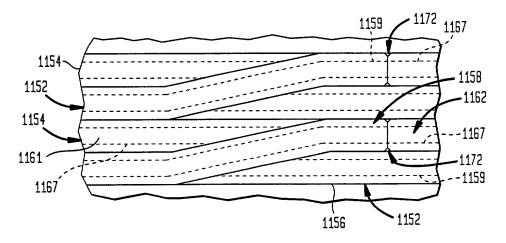


FIG. 18

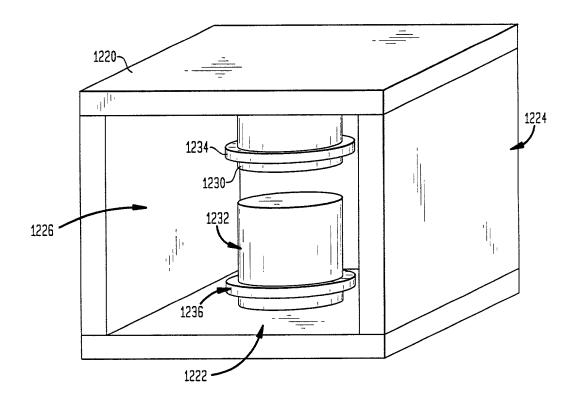

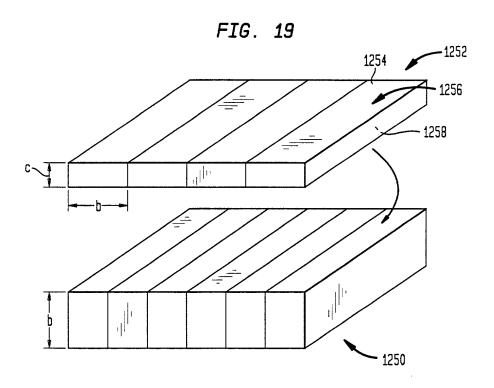

20/22

FIG. 20 **-** 1300 -1320 PRE PLACED COILS BED 2 1304 1302 1303 1304 c1305 1305 PATIENT MONITOR 600 BED 4 1328 206 600 -1301 - 600 PREP ROOM #2 PREP ROOM #1 · ※ BED N+1 ※ [BED 2] 1312 -BED 1 上600 600 PREP ROOM #3 PREP ROOM #4 READY LIGHTS 600 1312a 1314 ※ BED 3 S BED 4 600a --1324 1324 <u>1320</u> **EXIT EXIT ∃**600 PREP ROOM PREP ROOM #N+1 · ※ BED N BED N+1 CAMERA 0 ENTRANCE 600 1306 0 0 0 RECEPTION FILM PICKUP

T.V.

